

## **TECHNICAL FILE**

## Tracheostomy tube with low pressure cuff

523.30

Dated : 03-01-2022


1	1 Administrative information relating to the company		
1.1	Name : Vygon		
1.2	Address : 5 rue Adeline - 95440 Ecouen, France	<b>Fax :</b> + 33 (0)1 34 29 19 34 <b>E-mail :</b> questions@vygon.com <b>Website :</b> www.vygon.com	
1.3	Medical Device vigilance Representative : Laurent GUILLARDEAU	<b>Tel :</b> +33 (0)1 39 92 65 69 <b>Fax :</b> +33 (0)1 39 92 64 82 <b>E-mail :</b> quality@vygon.com	

2	Information about the device or equipment
2.1	Generic name : Tracheostomy tube
2.2	Commercial name : Tracheostomy tube with low pressure cuff
2.4	Medical Device Class : Ila Applicable regulation : 93/42/CEE in accordance with Appendix n° : Il Notified body N° : 0459 Medical Device Manufacturer : Vygon
2.5	Description of the device :   Tracheostomy tube transparent PVC tube with radiopaque line and low-pressure cuff.   Adjustable collar and tape.   This device is available in 5 sizes: 26Fr, 30Fr, 33Fr, 38Fr and 40Fr.



2.6	Packaging / Contain	ners			
	Code	Single unit packaging	Multi unit packaging	Minimum delivery quantity	Case
	523.30	1 (Supple blister )	1 (Carton box )	1 (Carton box )	90 (Case box )
	Single unit packaging				



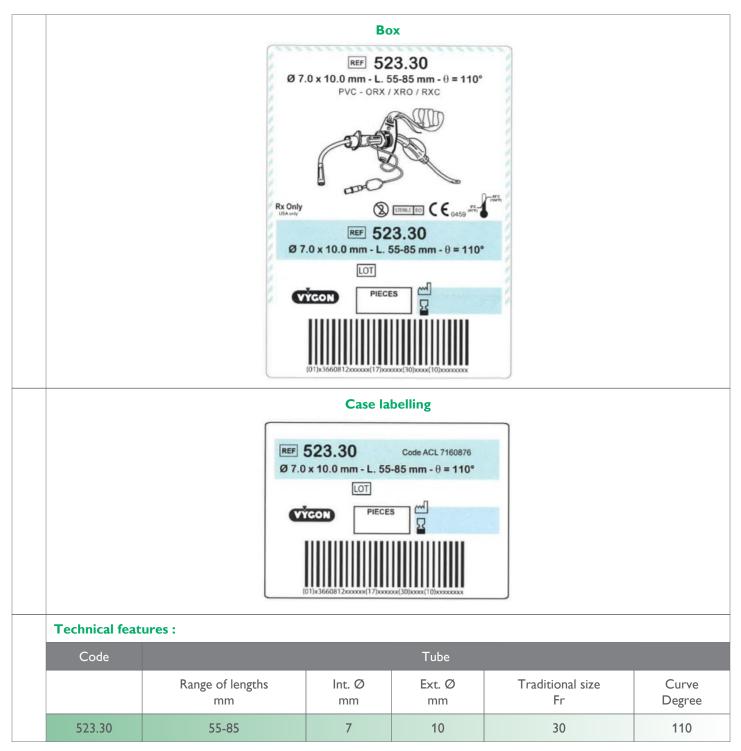



	vice and Accessories :	
COMPONENT	'S MARKER	MATERIALS
Canula tube	1	PVC
Cuff	2	PVC
Flange	3	PA
Nut	3	POM
Adapter	4	ABS
Inflation line	5	PVC
Tube / funnel	6	PVC
Таре	7	Polyester
Anti-return valv	re 8	Stain. steel/PVC/UP/Nitrile
	* 5	
<b>additional points :</b> Latex-free	are likely to come into contact with the patie	nt and/or administered products,
<b>additional points :</b> Latex-free DEHP-free		

3 Accessories



## Sterilization process

Sterile Medical Device : YES Sterilization made for the device : Ethylene oxide

5.1	<b>Normal conservation and storage conditions :</b> Storage environment temperature: between 5 and 40°C. Store protected from moisture and sunlight.
5.2	
5.3	Duration of product validity : 60 months

Security of use

## Instructions for use

7.1	
7.2	Indications : Tracheostomy
7.3	Precautions :
	Re-use of this device may change its mechanical or biological features and may cause device failure, allergic reaction or bacterial infections.
7.4	

8

Additional information relating to the product